

Login 

German  

Print 

Search

LCTech-en

Products

Automated Sample Preparation for Dioxins and PCB

DEXTech Plus

Results


Results

DIOXINS AND PCB


No Cross-Contamination

- Exchangeable columns
- Continuous rinsing of all parts that have got in contact with the sample
- No contact between sample and syringe pump


Reliable and Reproducible Results

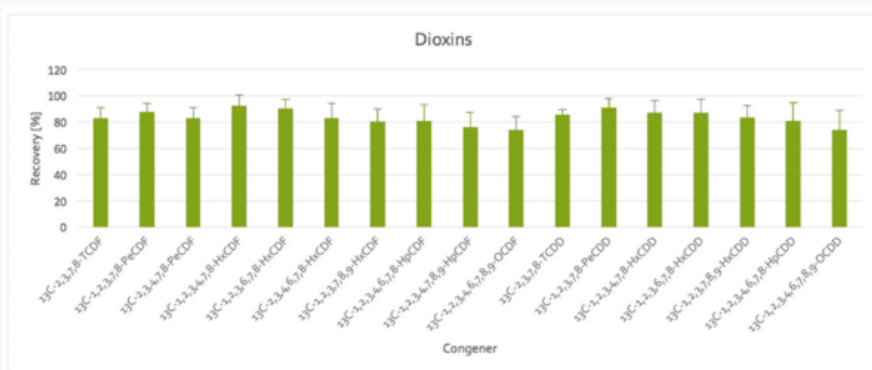

Results Dioxin Sources: Chemical and Veterinary Investigation Office Münsterland-Emscher-Lippe (governmental laboratory); LCTech Laboratory

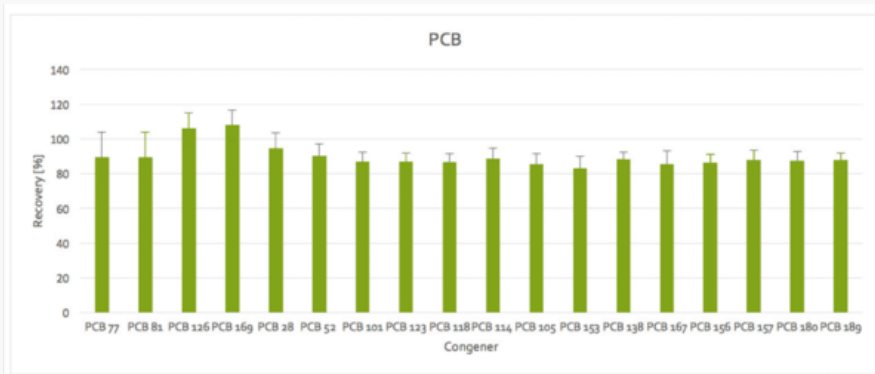

Results PCB Sources: Chemical and Veterinary Investigation Office Münsterland-Emscher-Lippe (governmental laboratory); LCTech Laboratory

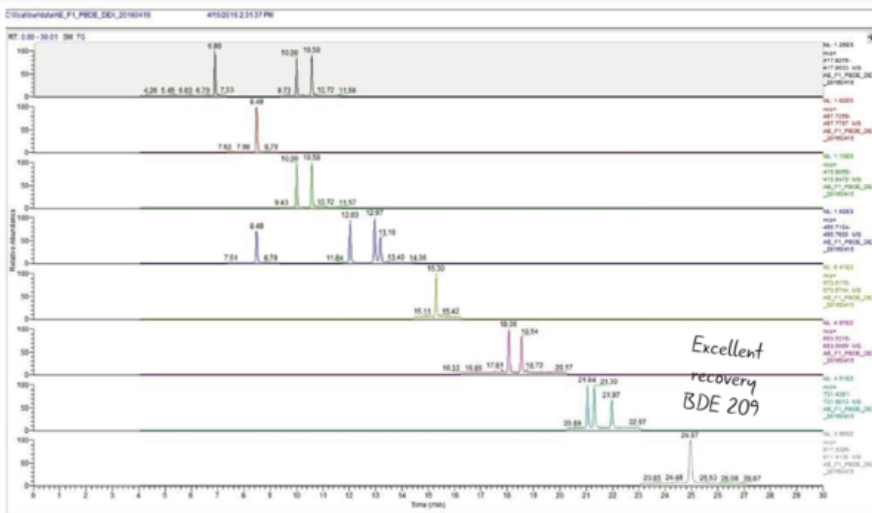

Clear signals, sharp separation, low background noise and excellent recoveries
Sources: Bavarian Health and Food Safety Authority (LGL-Oberschleißheim, governmental laboratory); LCTech Laboratory

Brochures

- [DEXTech product family brochure \(pdf | 3 MB\)](#)
- [DEXTech Plus brochure \(pdf | 2 MB\)](#)

Video

- [DEXTech Plus in action](#)

Application note

- [Automated clean-up of various brominated compounds: A breast](#)

[milk example \(pdf | 683 KB \)](#)

Press release

3,500 samples per year
throughput with the new
automated sample preparation
system for dioxin analysis
DEXTech Plus

© 2020 LCTech GmbH

[Disclaimer](#) |
[Data Security Statement](#) |
[Terms of Service](#) |
[Sitemap](#) |